

Ultra-sensitive NT-proBNP Test for Early Detection of Risk Factors Leading to Heart

Failure

Keum-Soo Song, Satish Balasaheb Nimse, Mukesh Digambar Sonawane, Shrikant Dashrat Warkad and Taisun Kim*

Institute for Applied Chemistry and Department of Chemistry, Hallym University, Chuncheon,

200-702, Korea; tskim@hallym.ac.kr

Supporting Information

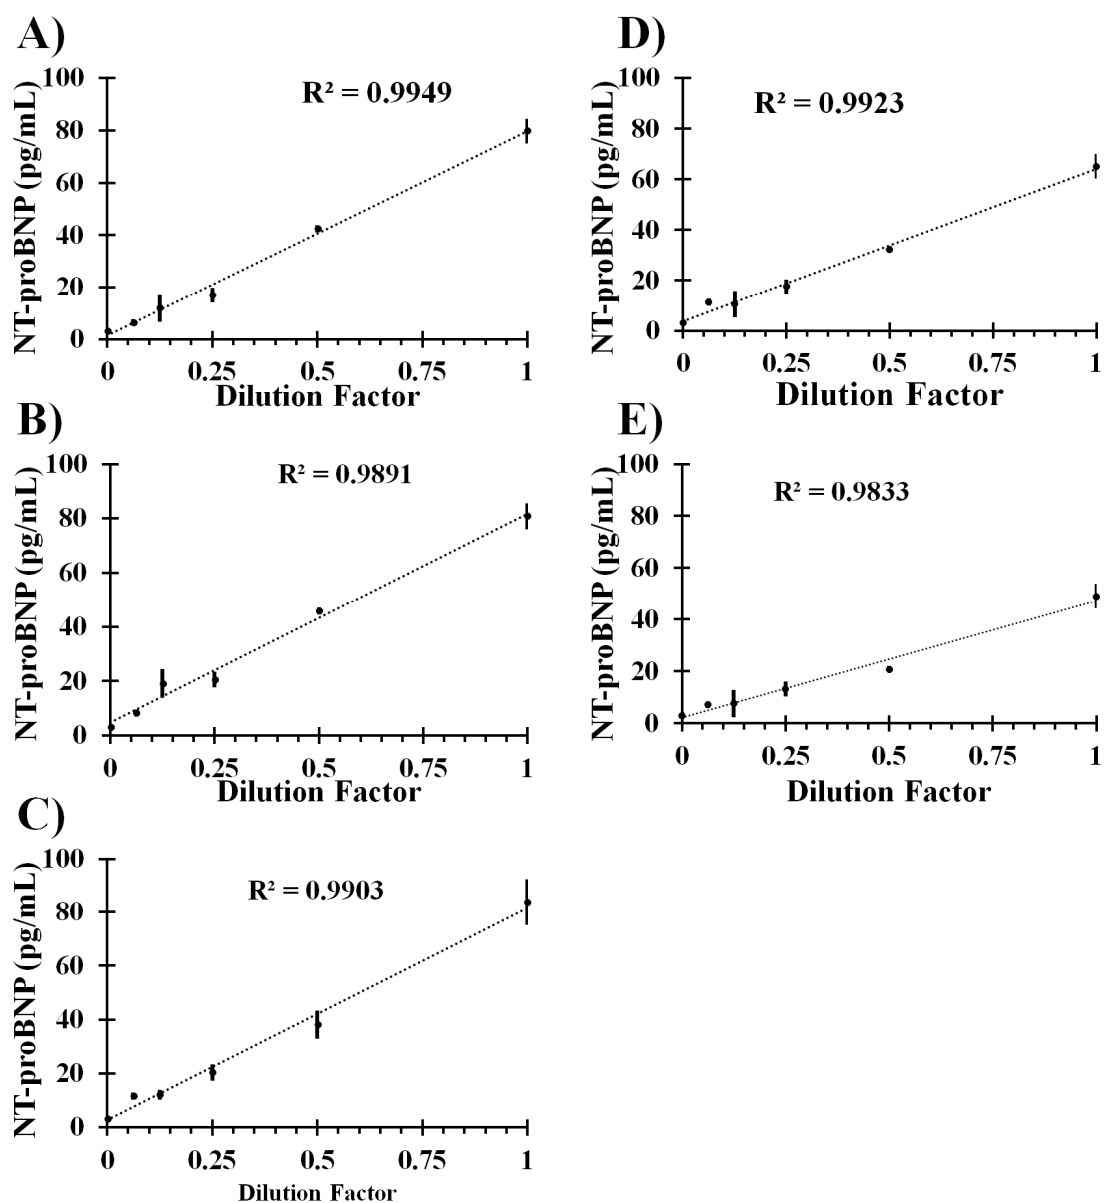


Figure S1: Linearity of test by dilution of non-spiked human serum samples containing A) 83.8pg/mL, B) 79.8 pg/mL, C) 65.2 pg/mL, D) 52.9 pg/mL, E) 49.1pg/mL NT-proBNP, respectively.