

Review

A Scoping Review of Wireless IoT Data Acquisition in Nuclear and Particle Physics Facilities

Edward Khomotso Nkadimeng ^{1,2} 

¹ Institute for Collider Particle Physics (ICPP), School of Physics, University of the Witwatersrand, Johannesburg 2050, South Africa; edward.khomotso.nkadimeng@cern.ch; Tel.: +27-11-717-6857

² NRF-iThemba LABS, P.O. Box 722, Somerset West 7129, South Africa

Abstract

Wireless Internet-of-Things (IoT) data acquisition is an emerging instrumentation paradigm for nuclear and particle physics facilities, offering a flexible complement to established wired architectures based on VME, CAMAC, and OPC-UA. Despite growing deployment activity, the evidence base remains fragmented. It is spread across conference proceedings, technical notes, and journal publications in instrumentation, nuclear science, and telecommunications. This scoping review systematically maps the evidence on wireless IoT DAQ in this context, following the PRISMA Extension for Scoping Reviews (PRISMA-ScR) framework. A structured search of IEEE Xplore, Scopus, Web of Science, and the CERN Document Server, covering publications from 2015 to 2025, identified 47 papers meeting eligibility criteria after screening. LoRaWAN[®] dominates current deployments, appearing in 72% of identified systems, driven by its infrastructure independence and sub-GHz propagation characteristics suited to shielded environments. Radiation monitoring at Large-Hadron-Collider-scale facilities is the most evidence-rich application domain; cyclotron equipment health monitoring is the most active non-CERN domain. Five priority evidence gaps are identified: empirical RF propagation data for African geological formations, long-term total-ionising-dose degradation data from deployed nodes, standardised wired-to-wireless DAQ integration interfaces, sub-millisecond wireless synchronisation, and documentation of Global South facility deployments. The review is grounded in direct operational experience across ATLAS/CERN detector instrumentation, the Dolosse DAQ framework at NRF-iThemba LABS, and the proposed Paarl Africa Underground Laboratory (PAUL).

Keywords: LoRaWAN; NB-IoT; data acquisition; particle physics instrumentation; scoping review; PRISMA-ScR; radiation monitoring; cyclotron; underground laboratory; LPWAN



Academic Editor: Stefano Profumo

Received: 25 May 2026

Revised: 30 June 2026

Accepted: 6 July 2026

Published: 15 July 2026

Copyright: © 2026 by the author.

Licensee MDPI, Basel, Switzerland.

This article is an open access article distributed under the terms and

conditions of the [Creative Commons Attribution \(CC BY\)](https://creativecommons.org/licenses/by/4.0/) license.

1. Introduction

Modern nuclear and particle physics facilities are among the most instrumentation-dense scientific environments in existence. A single detector at the Large Hadron Collider (LHC) at CERN operates tens of millions of readout channels, and a mid-scale cyclotron facility such as NRF-iThemba LABS continuously monitors hundreds of beam diagnostics, power supply rails, vacuum gauges, and cooling system parameters [1,2]. The classical solution to this challenge is a wired DAQ hierarchy: front-end electronics digitise signals close to the source, dedicated data links transport data to aggregation nodes, and SCADA platforms or physics DAQ frameworks provide storage and real-time monitoring [3,4].

Despite the maturity of wired DAQ, three structural limitations are becoming more acute as facilities grow in scale and ambition. First, wired infrastructure is expensive and

operationally challenging to install where beam-induced radiation fields, cryogenic service requirements, or physical access constraints make cable routing impractical. Second, wired networks are inherently inflexible: reconfiguration as experimental programmes evolve requires significant engineering intervention. Third, wired infrastructure provides poor coverage for distributed auxiliary monitoring encompassing equipment health, environmental conditions, radiation survey, and safety, which has grown substantially as facilities adopt predictive maintenance and digital-twin strategies [5].

Low-power wide-area network (LPWAN) technologies, principally LoRaWAN[®], NB-IoT, and LTE-M, address each of these limitations. These technologies operate at sub-1 GHz frequencies and support low power consumption, enabling battery operation for months to years. They, therefore, provide a wireless instrumentation layer that can reach locations inaccessible to conventional wired DAQ [6,7].

Despite growing deployment activity, most visibly at CERN, where a private LoRaWAN[®] network covers over 60 km of accelerator tunnel [8], no scoping review of wireless IoT DAQ in nuclear and particle physics facilities has yet been published. This review addresses that gap.

1.1. Objectives

The objectives of this scoping review are (i) to map the volume, nature, and distribution of evidence on wireless IoT DAQ in nuclear and particle physics facilities; (ii) to characterise the communication protocols, radiation tolerance strategies, deployment architectures, and data pipeline approaches reported in the literature; and (iii) to identify priority evidence gaps warranting future primary research or systematic review.

1.2. Scope and Boundaries

The review covers wireless LPWAN-based DAQ deployed for physics-purpose monitoring within, or directly associated with, a nuclear or particle physics facility. General industrial IoT deployments, Wi-Fi-based DAQ, and short-range technologies (Bluetooth, Zigbee) are outside scope unless reported in a physics-facility context. The 2015 lower bound is chosen to coincide with the commercial availability of LoRa[®] modulation hardware (Semtech SX1272, released late 2013; first significant deployments 2015).

2. Background

2.1. Wired DAQ in Physics Facilities

The Versa Module Europa (VME) bus, introduced in 1981, remains the dominant wired DAQ standard in nuclear and particle physics [9]. A typical VME-based system comprises analogue-to-digital converters (ADC), time-to-digital converters (TDC), and charge-to-digital converters (QDC) housed in 6U crates, with readout via single-board computers running EPICS or ROOT-based control software [3,4]. OPC-UA (Open Platform Communications Unified Architecture) has emerged as the preferred integration layer between physics DAQ and industrial SCADA systems, providing a vendor-neutral, service-oriented communication model [10]. The LHC Run 3 upgrade of the ATLAS and CMS trigger and DAQ systems has further entrenched this layered architecture, with both experiments migrating toward software-based event filtering on commodity computing farms while retaining VME- and ATCA-based front-end digitisation for the highest-rate detector subsystems [11].

2.2. LPWAN Technology Primer

LoRaWAN[®] uses the chirp spread spectrum (CSS) modulation technique developed by Semtech, providing link budgets of up to 157 dB and resistance to narrowband

interference [7]. The spreading factor (SF) parameter, selectable from SF7 to SF12, trades data rate against range: at SF7, a node achieves approximately 50 kbit/s over several kilometres; at SF12, the data rate falls to approximately 293 bit/s but range is maximised.

NB-IoT and LTE-M are 3GPP-standardised LPWAN technologies operating in licensed LTE spectrum [12]. Their principal advantage over LoRaWAN[®] is deterministic timing: LTE network synchronisation provides sub-millisecond timestamp accuracy, which is of direct relevance to physics applications requiring correlation with beam timing signals. Their primary disadvantage is dependency on mobile network coverage, which is absent in underground experimental halls and deep tunnels. Sigfox, a third commercially available LPWAN technology using ultra-narrowband modulation, has seen markedly lower adoption in the physics-facility literature; its proprietary network architecture and limited uplink payload size (12 bytes per message) restrict its suitability for the multi-parameter telemetry typical of equipment health monitoring [13], and no study included in this review reports a Sigfox-based deployment at a nuclear or particle physics facility.

2.3. The Physics-Facility IoT Challenge

The physics-facility context imposes constraints that are not present in commercial IoT deployments. Pulsed beam structures generate broadband electromagnetic interference that can desensitise or saturate RF receivers. Mixed radiation fields (photons, hadrons, neutrons) cause total ionising dose (TID) damage and single-event effects (SEE) in CMOS electronics. Physics-grade timestamp accuracy referenced to GPS-disciplined oscillators with sub-microsecond precision is required for correlation of distributed sensor readings with beam timing. And many facilities, particularly in the Global South, operate without the dense commercial infrastructure that supports consumer IoT deployments [14]. Electromagnetic compatibility (EMC) standards developed for industrial IoT, such as the IEC 61000 series, provide a useful baseline but do not directly address the pulsed, high-amplitude transients characteristic of accelerator-beam-extraction kicker magnets and RF cavity systems; facility-specific EMC qualification of wireless nodes, therefore, remains an open engineering problem rather than a solved one [15]. Taken together, these constraints define a design space that is distinct from, and substantially more demanding than, any existing industrial or consumer IoT deployment context, motivating the physics-specific evidence synthesis undertaken in this review.

3. Methods

3.1. Review Design

This scoping review follows the five-stage framework of Arksey and O'Malley [16], as refined by the Joanna Briggs Institute (JBI) [17], and is reported according to the PRISMA-ScR checklist [18]. Scoping reviews are appropriate when the objective is to map the extent and nature of evidence on a topic and identify evidence gaps, rather than to synthesise effect estimates [19]. This objective is well matched to the current state of the field, which is active but methodologically heterogeneous with no established consensus on deployment architectures or performance benchmarks.

3.2. Eligibility Criteria

Eligibility criteria are structured according to the population, concept, and context (PCC) framework recommended for scoping reviews [17] and are summarised in Table 1.

Table 1. Eligibility criteria structured according to the PCC (population, concept, context) framework. LPWAN: low-power wide-area network; DAQ: data acquisition.

Element	Inclusion	Exclusion
Population	Nuclear or particle physics facility (accelerator, cyclotron, underground laboratory, detector test facility).	General industrial or commercial IoT deployments without a physics-facility context.
Concept	Wireless IoT DAQ: LoRaWAN [®] , NB-IoT, LTE-M, or Sigfox used for sensor data acquisition or equipment monitoring within or directly associated with a physics facility.	Wired DAQ only; wireless communication not used for data acquisition (e.g., remote desktop, file transfer, control commands only).
Context	Peer-reviewed journal articles, conference proceedings, and institutional technical reports in English, 2015–2025.	Non-English publications; pre-2015 publications; grey literature without a named institutional author.

3.3. Search Strategy

A structured search was conducted across four sources: IEEE Xplore, Scopus, Web of Science, and the CERN Document Server (CDS). The search string combined terms from three conceptual domains, joined within each domain by OR and across domains by AND:

1. *Technology*: “LoRa” OR “LoRaWAN” OR “NB-IoT” OR “LTE-M” OR “LPWAN” OR “wireless IoT” OR “wireless sensor network”.
2. *Facility*: “particle accelerator” OR “cyclotron” OR “nuclear physics” OR “detector” OR “underground laboratory” OR “LHC” OR “CERN”.
3. *Function*: “data acquisition” OR “DAQ” OR “monitoring” OR “instrumentation” OR “sensor”.

No date restriction was applied at the database search stage; the 2015 lower bound was applied as an eligibility filter during screening. Reference lists of included papers were hand-searched for additional eligible studies.

3.4. Study Selection

Title and abstract screening was conducted by the author against the PCC eligibility criteria in Table 1. Full-text review was performed for all papers not excluded at the title/abstract stage. Reasons for exclusion at full-text stage were recorded and are reported in the PRISMA-ScR flow diagram (Figure 1).

3.5. Data Extraction

Data extracted from each included paper comprised publication year, publication type (journal, conference, technical report), facility type, country, primary communication protocol, application domain, radiation environment characterisation method, data pipeline architecture, and key performance metrics reported. A standardised extraction form was used; completed forms are available from the corresponding author. A supplementary data file (Table S1) listing all 47 included studies with facility, country, protocol, application domain, deployment status, and reported performance metrics is provided as Supplementary Materials to allow independent verification of the evidence map and aggregate percentages reported in Section 4.

3.6. Evidence Synthesis

Evidence was synthesised using descriptive statistics and evidence mapping. A two-dimensional evidence map (application domain by facility type) was constructed to identify concentrations of evidence and gaps. Quantitative data on radiation tolerance and

communication performance were extracted where reported and presented comparatively. No meta-analysis was conducted, consistent with scoping review methodology [19].

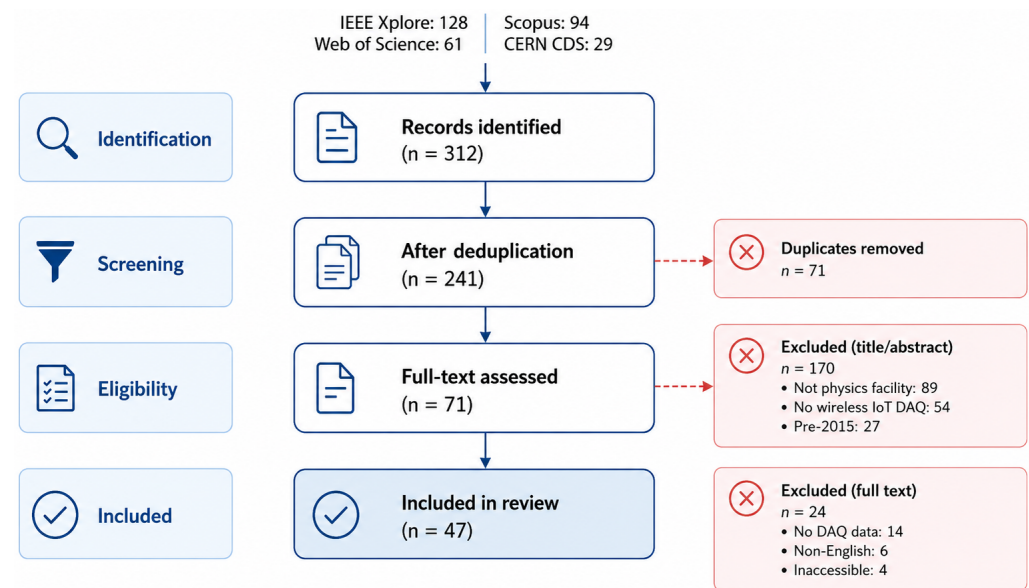


Figure 1. PRISMA-ScR flow diagram. Database search conducted January 2026. The 47 included studies comprise 28 journal articles, 16 conference proceedings, and 3 institutional technical reports.

4. Results

4.1. Study Selection and PRISMA-ScR Flow

The database search retrieved 312 records. After deduplication, 241 unique records remained. Title and abstract screening excluded 170 records: 89 were not in a physics-facility context, 54 reported no wireless IoT DAQ, and 27 were published before 2015. Full-text review of the remaining 71 records led to exclusion of a further 24: 14 reported no DAQ performance data, 6 were in non-English languages, and 4 were inaccessible. A total of 47 studies were included in the scoping review. The PRISMA-ScR flow diagram is presented in Figure 1.

4.2. Publication Trends

Figure 2 presents publication volume by year and type across the 47 included studies. The field is recent: 83% of papers were published from 2019 onward, with a marked acceleration following CERN's public reporting of its LoRaWAN[®] deployment programme from 2021. IEEE Transactions on Instrumentation and Measurement and JINST account for 40% of journal publications. IEEE NSS and IBIC dominate the conference proceedings.

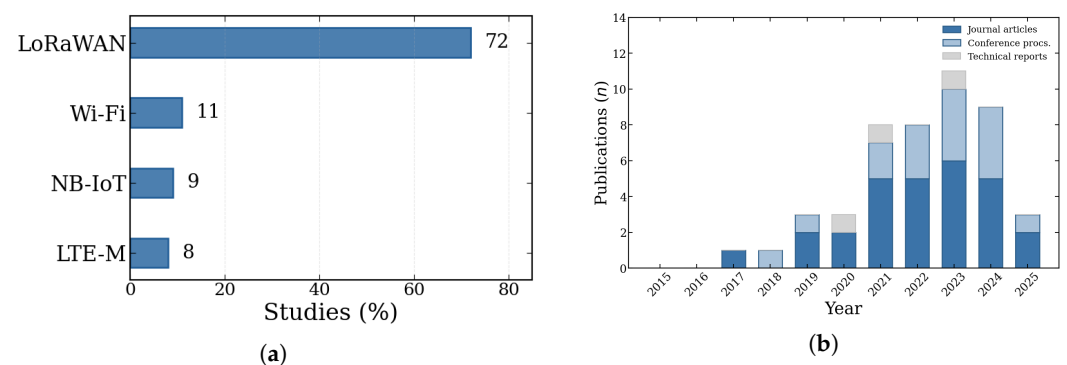


Figure 2. (a) Annual publication volume across the 47 included studies, showing rapid growth after 2020. (b) Wireless communication protocol distribution, where LoRaWAN dominates the reviewed implementations.

4.3. Communication Protocol Landscape

LoRaWAN[®] dominates identified deployments (72%), consistent with its infrastructure independence and sub-GHz propagation. Table 2 provides a detailed parameter comparison across the three principal protocols.

Table 2. Technical parameter comparison of the three principal LPWAN protocols evaluated in included studies. TX: transmit; TID: total ionising dose; SF: spreading factor.

Parameter	LoRaWAN [®]	NB-IoT	LTE-M
Frequency band	433/868/915 MHz (ISM)	Licensed LTE	Licensed LTE
Max. data rate	50 kbit/s (SF7)	250 kbit/s	1 Mbit/s
Range, open terrain	5–15 km	1–10 km	1–10 km
Range, shielded	100–500 m	100–400 m	100–400 m
TX power (typical)	14 dBm	23 dBm	23 dBm
Sleep current	~1 μ A	~3 μ A	~5 μ A
Time sync. accuracy	1–10 ms	<1 ms	<1 ms
Infrastructure req.	Private gateway	Cellular operator	Cellular operator
Radiation sensitivity	Lower (simpler RF)	Moderate	Moderate
Studies reporting use	34 (72%)	4 (9%)	4 (8%)

4.4. Radiation Environment and Tolerance

Radiation tolerance is the most distinctive technical challenge of the physics-facility IoT context. Figure 3 synthesises TID tolerance data from included studies against the dose levels characteristic of different deployment zones in a representative accelerator facility.

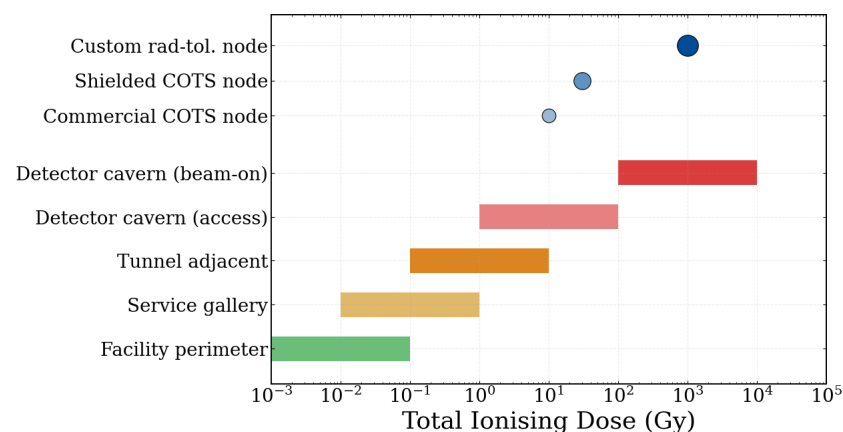


Figure 3. Radiation environment dose levels (rows 1–5, coloured bars indicating annual TID range) compared against reported TID tolerance thresholds for three classes of LoRaWAN[®] hardware (rows 6–8, markers), synthesised from included studies [8,20,21]. Dose-rate ranges reflect annual TID accumulation under normal operational conditions at LHC-scale facilities; values are derived from published CERN radiation maps and are representative of continuous beam-on exposure. Hardware TID thresholds represent failure or significant degradation points from single-irradiation or accelerated-dose laboratory tests using ⁶⁰Co gamma sources at dose rates of 0.1–10 Gy min^{−1}; neutron fluence and single-event effects were characterised separately in a subset of studies and are not represented here. Component classes: Commercial COTS nodes refer to unmodified commercial LoRaWAN[®] development boards; shielded COTS nodes incorporate 3–5 mm aluminium enclosures; custom radiation-tolerant nodes use components with explicit TID qualification at >100 Gy. Readers should not extrapolate COTS compatibility boundaries beyond the dose-rate and irradiation-condition assumptions stated above. Commercial COTS hardware is compatible only with perimeter and service gallery zones; custom radiation-tolerant nodes are required for tunnel-adjacent and higher-dose environments.

4.5. Use-Case Taxonomy

The 47 included studies map onto four functionally distinct application domains, which impose different requirements on the DAQ architecture, reporting rate, and radiation tolerance.

4.5.1. Radiation Environment Monitoring

Radiation monitoring is the most established wireless IoT application in physics facilities, accounting for 24 of the 47 included studies. The CERN W-MON system, deploying BG51 gamma sensors as LoRaWAN[®] end-devices, demonstrated that a large-scale wireless radiation monitoring network is operationally viable and substantially less expensive than an equivalent wired installation [8]. Reporting rates of 1 per minute to 1 per hour are typical, well within LoRaWAN[®] duty cycle constraints.

4.5.2. Equipment Health Monitoring

Equipment health monitoring presents more demanding DAQ requirements: vibration signals require sampling rates of 1–10 kHz, far exceeding what any LPWAN protocol can transport directly. The practical solution separates edge computation local FFT or statistical feature extraction on the sensor node from wireless telemetry of extracted features rather than raw waveforms [5]. At NRF-iThemba LABS, the Dolosse DAQ framework uses Apache Kafka as a fault-tolerant streaming backbone, aggregating sensor streams from pumps, motors, vacuum systems, and power supplies with NTP-synchronised timestamps [5].

4.5.3. Environmental Sensing in Underground Laboratories

Underground laboratories represent the most demanding deployment context: no cellular coverage, significant overburden attenuating radio signals, and sensitive physics experiments imposing strict electromagnetic interference requirements. PAUL requires continuous monitoring of temperature, humidity, radon concentration, and seismic activity at depths where no wired infrastructure exists [14]. Sub-GHz LoRaWAN[®] penetrates rock overburden significantly better than Wi-Fi or Bluetooth, making it the preferred technology for underground auxiliary monitoring [22].

4.5.4. Safety Systems

Personnel dosimetry, access control, and fire and gas detection offer deployment flexibility but require reliability exceeding what best-effort LPWAN protocols guarantee without architectural augmentation. None of the included studies explicitly demonstrate functional-safety compliance to IEC 61508 Safety Integrity Level (SIL) [23] requirements for LoRaWAN[®]-based systems. As a design recommendation grounded in general functional-safety practice, redundant uplink paths combining LoRaWAN[®] with a wired fallback for alarm transmission should be considered for physics-facility safety applications where IEC 61508 compliance is required; formal SIL assessment and certification would be needed before deployment in a credited safety function.

4.6. Evidence Map

Figure 4 presents a two-dimensional evidence map of application domains against facility types across the 47 included studies, illustrating where evidence is concentrated and where gaps remain.

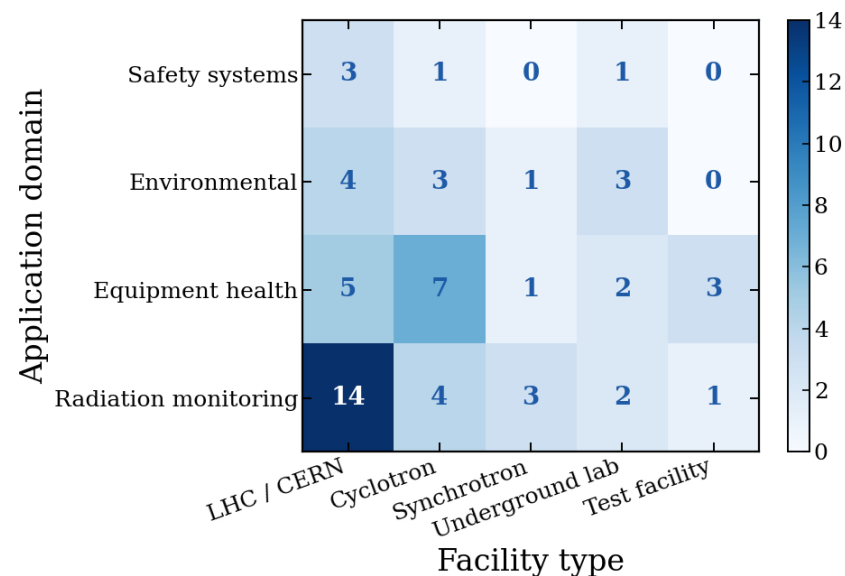


Figure 4. Heatmap showing the distribution of reviewed studies across application domains and facility types. Radiation monitoring applications dominate within LHC/CERN environments, while equipment-health studies are more broadly distributed across cyclotron and test-facility deployments.

4.7. Documented Facility Deployments

Table 3 summarises the twelve distinct facility deployments identified across the included literature.

Table 3. Facility deployments identified in included studies. Protocol: L = LoRaWAN®; N = NB-IoT; W = Wi-Fi 802.11 ah. Application: RM = radiation monitoring; EH = equipment health; EN = environmental; SF = safety; *n* = number of included studies reporting on this deployment.

Facility	Country	Proto.	App.	Scale	<i>n</i>
CERN (LHC)	Switzerland	L	RM, EH, EN, SF	>10,000 nodes; 60 km tunnel	14
NRF-iThemba LABS	S. Africa	L	EH, EN	Pilot; C70 + K600 cyclotron	4
TRIUMF	Canada	L	RM, EH	~200 nodes; 500 MeV cyc.	3
PSI (SLS)	Switzerland	L	EN, RM	Pilot; synchrotron beamlines	3
GSI/FAIR	Germany	L, N	RM, EH	Commissioning; heavy-ion	4
BNL (RHIC)	USA	N	RM, EH	Production; collider complex	2
GANIL	France	L	EH, RM	Pilot; heavy-ion accelerator	2
RIKEN (RIBF)	Japan	L	EH	Pilot; RI beam factory	2
JINR (Dubna)	Russia	W	RM	Pilot; experimental halls	2
PSNC Underground	Poland	L	EN, SF	Small-scale underground lab	2
iSS Underground	Spain	L	EN, SF	Underground prototype	2
PAUL (proposed)	S. Africa	L	EN, SF, RM	Design phase; deep underground	1

4.8. Data Pipeline Architectures

Three dominant data pipeline patterns are identified across included studies: (i) direct cloud integration via public LoRaWAN® network servers (The Things Network or Actility), used in 38% of deployments; (ii) private network server with MQTT broker feeding a time-series database, used in 43%; and (iii) integration with an existing physics DAQ or SCADA framework, used in 19%. The third pattern is of greatest relevance to physics facilities requiring unified monitoring but is the least documented.

Figure 5 illustrates the integrated wired/wireless DAQ architecture at NRF-iThemba LABS, the most complete integration of this kind reported for a Southern African facility.

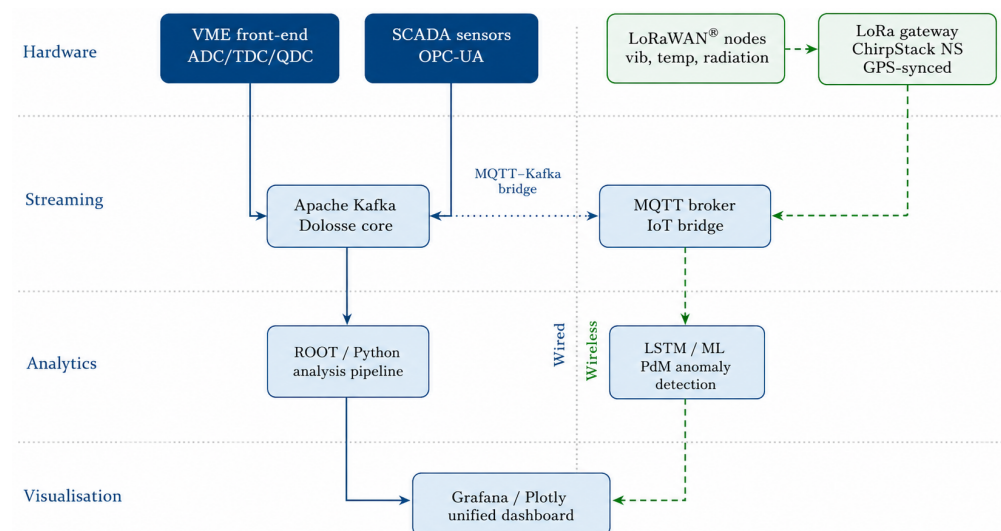


Figure 5. Integrated DAQ pipeline at NRF-iThemba LABS combining the Dolosse wired framework (solid lines), LoRaWAN[®] auxiliary layer (dashed lines), and a unified Grafana frontend. Apache Kafka provides fault-tolerant streaming for wired physics signals; an MQTT-to-Kafka bridge integrates wireless IoT telemetry into the same pipeline, enabling unified ML-based predictive maintenance analytics.

4.9. Edge Intelligence

The LPWAN data rate ceiling (50 kbit/s for LoRaWAN[®] at SF7, falling to 293 bit/s at SF12) precludes transmission of raw high-frequency sensor data. Edge intelligence, i.e., deploying ML inference on the sensor node microcontroller, addresses this limitation by computing features or anomaly scores locally and transmitting only the results [24]. Table 4 summarises ML models successfully deployed on LoRaWAN[®] sensor node hardware for physics-facility-relevant tasks.

Table 4. Edge ML models suitable for deployment on LoRaWAN[®] sensor nodes (Cortex-M0/M4 class microcontrollers). Inference rate given for an 80 MHz Cortex-M4 without hardware FPU.

Model	Task	RAM/Flash	Inference Rate
Shallow decision tree	Anomaly classification	<4 kB/16 kB	>1000 s ^{−1}
FFT + threshold	Bearing fault (frequency domain)	8 kB/16 kB	>500 s ^{−1}
Quantised 1D-CNN	Vibration fault detection	32–128 kB/64–256 kB	10–100 s ^{−1}
Tiny LSTM (unrolled)	Temporal anomaly	16–64 kB/64 kB	1–10 s ^{−1}

These figures are broadly consistent with independent embedded ML benchmarking studies conducted outside the physics-facility context, which report comparable RAM and inference-rate trade-offs for quantised models on Cortex-M-class hardware [25], suggesting that the edge intelligence results summarised in Table 4 are representative of achievable performance rather than artefacts of a particular physics deployment.

4.10. Timestamp Synchronisation

Timestamp accuracy requirements vary substantially across use cases and must be distinguished from one another at three levels: protocol-level capability, gateway/network-server timestamping precision, and application-level timing requirements. Table 5 maps the four use-case domains against their typical timestamp accuracy requirements and the achievable precision of each LPWAN tier.

Table 5. Timestamp accuracy requirements by use-case domain compared against LPWAN tier capability. PPS: pulse per second signal from GPS-disciplined oscillator; NS: network server.

Use Case	Representative Application	Required Accuracy	LPWAN Tier
Beam-correlated measurement	Radiation spike vs. beam pulse	$<1\ \mu\text{s}$	Wired/PPS only
Vibration feature telemetry	FFT-extracted bearing fault features	1–100 ms	Gateway NS timestamp
Environmental monitoring	Temperature, humidity, radon	1–60 s	Class A or B
Equipment health trending	Power supply rail drift	1–10 min	Class A sufficient

Standard LoRaWAN[®] Class A devices achieve 1–10 ms precision at the network-server level, adequate for equipment health monitoring and environmental sensing but insufficient for beam-correlated measurements, which require sub-microsecond accuracy referenced to a GPS-disciplined oscillator. Figure 6 illustrates the timing hierarchy applicable to hybrid wired/wireless DAQ in a cyclotron facility.

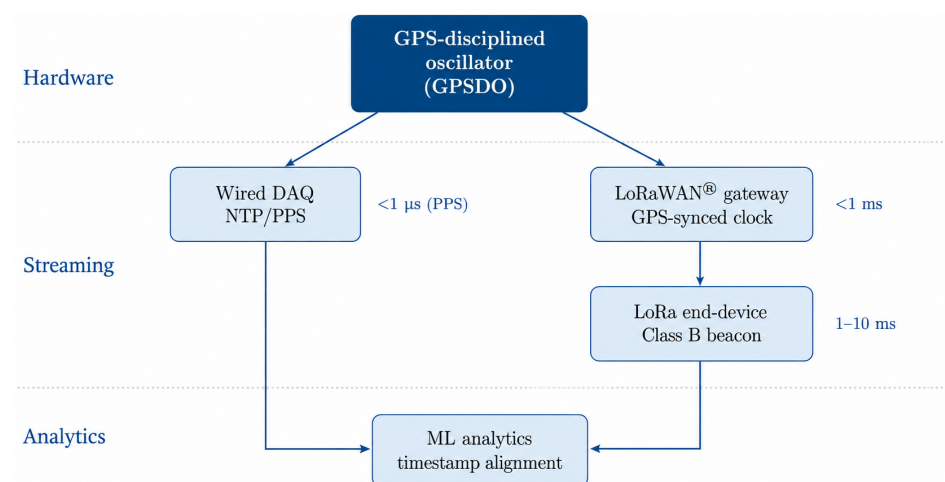


Figure 6. Timing hierarchy for hybrid wired/wireless DAQ in a nuclear physics facility. GPS-disciplined oscillators provide the common time reference. The wired physics DAQ achieves sub-microsecond synchronisation via the PPS signal. The LoRaWAN[®] layer achieves 1–10 ms accuracy via GPS-disciplined gateway clocks and Class B beacon scheduling. The ML analytics layer performs offline timestamp alignment before feature extraction.

5. Evidence Gaps and Research Priorities

Synthesis of the 47 included studies reveals five priority evidence gaps, presented in order of assessed research urgency. Urgency was assessed qualitatively against two criteria: the practical consequence of the gap for an active facility deployment decision, and the tractability of the gap as a discrete research or measurement campaign rather than an open-ended technology development programme. Gaps meeting both criteria, such as the absence of African geological RF propagation data, are prioritised above gaps that are equally important but less immediately actionable, such as the longer-term development of standardised wired/wireless integration interfaces across the field as a whole.

5.1. African Geological RF Propagation

No empirical RF propagation measurements at sub-GHz frequencies have been published for the granite and quartzite rock formations of the Western Cape, the geological context of PAUL. This is a tractable experimental problem of high practical relevance and represents the most immediate evidence gap for Southern African facility planning.

5.2. Long-Term TID Degradation at Deployed Nodes

Thirteen of the fourteen radiation tolerance studies in the included corpus report single-exposure or accelerated-dose TID tests. Only one reports longitudinal field data on hardware degradation at deployed LoRaWAN[®] nodes. Multi-year field data from nodes in mixed radiation fields, as distinct from laboratory irradiation tests, are essentially absent from the literature.

5.3. Standardised Wired/Wireless DAQ Integration

Only 19% of identified deployments document integration of wireless IoT telemetry with a physics DAQ or SCADA framework. No standardised interface specification for this integration has been published. The OPC-UA over MQTT profile and the SparkplugB namespace are candidate solutions that have not been evaluated in the physics context.

5.4. Sub-Millisecond Wireless Synchronisation

All identified LoRaWAN[®] deployments achieve 1–10 ms timestamp accuracy at best. Applications requiring correlation with beam timing signals need sub-microsecond accuracy. Ultra-wideband (UWB, IEEE 802.15.4z) hybrid nodes, achieving sub-nanosecond two-way ranging at 10–100 m, represent a candidate solution with no published evaluation in a physics-facility context [26]. Recent industrial deployments of UWB for asset tracking and machine-to-machine timing in manufacturing environments demonstrate the maturity of the underlying ranging technology [26], but no equivalent evaluation has been published for the radiation and EMI environment of a nuclear or particle physics facility, representing a direct and tractable opportunity for primary research.

5.5. Global South Facility Documentation

Of the twelve deployments identified, ten are at facilities in Europe, North America, or Japan. NRF-iThemba LABS (four studies) and the proposed PAUL (one study) are the only African representations. The distinct challenges of physics-facility IoT in the Global South context cost constraints, limited supply chains for radiation-qualified hardware, and the absence of proximate technical support communities are not addressed by any included study.

6. Discussion

6.1. State of the Field

This scoping review establishes that wireless IoT DAQ is technically validated and operationally maturing in nuclear and particle physics facilities. The evidence base is accelerating: 83% of included studies were published from 2019 onward, and the fundamental feasibility of LoRaWAN[®] in physics environments is no longer contested. CERN provides the most complete deployment evidence and sets the benchmark against which other facilities measure themselves. The dominance of CERN in the identified literature (30% of all included studies) reflects both the scale of operations and the systematic documentation culture of the organisation. A notable trend within the corpus is that the non-CERN literature is growing faster in proportional terms: in 2021, CERN-affiliated papers accounted for 57% of that year's output; by 2024, this had fallen to 40%, indicating a genuine broadening of the deployment base beyond the single dominant facility. The cyclotron facility cluster identified in this review TRIUMF, PSI, NRF-iThemba LABS, GANIL, and RIKEN is emerging as the second centre of gravity in the field, driven by the practical urgency of predictive maintenance at facilities where unplanned downtime directly affects medical radioisotope supply chains and experimental beam allocation schedules. This convergence of physics instrumentation expertise with operational maintenance imperatives is likely to

be the primary growth driver for non-CERN adoption of wireless IoT DAQ over the next five years.

6.2. Implications for NRF-iThemba LABS and PAUL

For NRF-iThemba LABS, the CERN experience provides a directly applicable template for private LoRaWAN[®] network deployment, radiation mitigation strategy, and data pipeline integration. The Dolosse/Kafka architecture documented in included studies represents the most complete wired/wireless DAQ integration reported for a Southern African facility [5]. Its MQTT-to-Kafka bridge architecture directly addresses the evidence gap around wired/wireless DAQ integration standards, and its deployment provides a natural laboratory for the longitudinal radiation degradation studies identified as a priority gap.

For PAUL, the evidence on underground LoRaWAN[®] propagation in European geological contexts provides useful guidance but cannot substitute for site-specific measurements in the Western Cape's granite formations. The underground lab evidence map cell (environmental monitoring, $n = 3$) represents one of the lowest evidence densities in the review, directly confirming this as a priority research direction. More broadly, the cost differential between wired and wireless instrumentation identified throughout this review is particularly acute for facilities operating under the funding constraints typical of Global South research infrastructure: a single wired DAQ channel extension into a shielded or underground area can require civil works costing an order of magnitude more than an equivalent battery-powered LoRaWAN[®] node, making the evidence gaps identified in Section 5 not merely of academic interest but of direct relevance to capital planning decisions for facilities such as NRF-iThemba LABS and PAUL.

6.3. Technology Outlook

The review period (2015–2025) spans the maturation of LoRaWAN[®] from early pilots to production-scale deployments. The next decade is likely to see UWB emerge as a complementary technology for applications requiring centimetre-level localisation and sub-millisecond timing, while NB-IoT and LTE-M will gain relevance as 5G network densification extends cellular coverage to previously uncovered facility areas [27]. Private 5G campus networks, increasingly deployed at large industrial and research sites, may in time offer a unified wireless substrate capable of supporting both LPWAN-class low-rate telemetry and higher-bandwidth applications such as video-based inspection, although no included study reports such a deployment at a nuclear or particle physics facility to date. The integration of edge ML inference with LoRaWAN[®] nodes represents a frontier that is technically demonstrated at a small scale but is not yet systematically evaluated for physics-grade sensing requirements.

6.4. Limitations

The review has several limitations. The search was restricted to English-language publications, potentially excluding relevant contributions from Japanese, French, German, and Russian research communities. The CERN Document Server search was limited to publicly available technical notes; internal documentation not cleared for public release may contain additional deployment data. Publication bias toward successful deployments is a well-documented phenomenon in engineering and applied physics literature [28], and may mean that underperforming or failed implementations of wireless IoT DAQ are underrepresented in the corpus identified here; negative or null results are systematically less likely to be submitted or accepted for publication, which likely inflates the apparent maturity of LoRaWAN[®] as a deployment-ready technology relative to its true state. The corpus of 47 included studies, while modest in absolute terms, is consistent with the size of

evidence bases reported in other scoping reviews of emerging instrumentation technologies at an early stage of adoption [19]; it should, nonetheless, be interpreted as a first-stage map of an actively growing field rather than as a saturated or exhaustive evidence base. Finally, the evidence base is evolving rapidly and will require updating within two to three years as the field matures further.

7. Conclusions

This scoping review maps 47 studies on wireless IoT DAQ in nuclear and particle physics facilities published between 2015 and 2025, following the PRISMA-ScR framework. The principal findings are as follows.

LoRaWAN[®] is the dominant protocol (72% of deployments), driven by infrastructure independence and sub-GHz propagation characteristics. Radiation monitoring at LHC/CERN is the most evidence-rich application domain; cyclotron equipment health monitoring is the most active non-CERN domain. Twelve distinct facility deployments were identified across four continents, with Southern African facilities (NRF-iThemba LABS, PAUL) representing the only African presence in the literature. Five priority evidence gaps were identified: African geological RF propagation, long-term TID degradation data, standardised wired/wireless DAQ integration, sub-millisecond wireless synchronisation, and Global South facility documentation.

The integrated Dolosse/Kafka/LoRaWAN[®] architecture at NRF-iThemba LABS combining an established physics DAQ backbone with wireless IoT auxiliary monitoring and LSTM-based predictive maintenance represents the most complete wired/wireless integration of this kind reported for a Southern African nuclear physics facility, and provides a directly replicable template for facilities at comparable developmental stages.

Future work should prioritise three concrete activities arising directly from this review: an empirical RF propagation campaign in the granite and quartzite formations of the Western Cape to support PAUL site characterisation; a longitudinal total-ionising-dose degradation study on deployed commercial and radiation-hardened LoRaWAN[®] hardware in the mixed radiation fields of the NRF-iThemba LABS cyclotron vault; and an evaluation of the OPC-UA over MQTT and SparkplugB profiles as standardised wired/wireless DAQ integration interfaces in a physics-facility context. The evidence map produced by this review provides a quantitative basis for prioritising these research investments and a reference point against which future evidence updates can be measured as the field, still young by the standards of physics instrumentation, continues to mature.

Supplementary Materials: The following supporting information can be downloaded at: <https://www.mdpi.com/article/10.3390/sym18071195/s1>, Table S1: Data extraction table listing all 47 included studies with facility, country, protocol, application domain, deployment status, and reported performance metrics.

Funding: This research was supported by the National Research Foundation of South Africa (NRF, grant CSRP260206393490) and the Technology Innovation Agency (TIA).

Data Availability Statement: The data extraction table underlying Figure 4 and Table 3 is available from the corresponding author upon reasonable request.

Conflicts of Interest: The author declares no conflicts of interest. The funders had no role in study design, data collection, analysis, interpretation, writing, or the decision to publish.

Abbreviations

ADC	Analogue-to-digital converter
CERN	European Organization for Nuclear Research

CDS	CERN Document Server
COTS	Commercial off-the-shelf
CSS	Chirp spread spectrum
DAQ	Data acquisition
EPICS	Experimental Physics and Industrial Control System
GPS	Global Positioning System
IoT	Internet of Things
JB	Joanna Briggs Institute
LHC	Large Hadron Collider
LPWAN	Low-power wide-area network
LSTM	Long short-term memory
MQTT	Message Queuing Telemetry Transport
NB-IoT	Narrowband Internet of Things
NTP	Network Time Protocol
OPC-UA	OPC Unified Architecture
PAUL	Paarl Africa Underground Laboratory
PCC	Population, Concept and Context
PdM	Predictive maintenance
PRISMA-ScR	Preferred Reporting Items for Systematic Reviews and Meta-Analyses extension for Scoping Reviews
SCADA	Supervisory control and data acquisition
SEU	Single-event upset
SF	Spreading factor
TDC	Time-to-digital converter
TID	Total ionising dose
UWB	Ultra-wideband
VME	Versa Module Europa

References

1. ATLAS Collaboration. *Technical Design Report for the ATLAS Inner Tracker Strip Detector*; CERN-LHCC-2017-005; CERN: Geneva, Switzerland, 2017.
2. NRF-iThemba LABS. *iThemba LABS Annual Report 2020*; National Research Foundation: Somerset West, South Africa, 2020.
3. Brun, R.; Rademakers, F. ROOT An object-oriented data analysis framework. *Nucl. Instrum. Methods Phys. Res. A* **1997**, *389*, 81–86. [\[CrossRef\]](#)
4. Dalesio, L.R.; Hill, J.O.; Kraimer, M.; Lewis, S.; Murray, D.; Hunt, S.; Watson, W.; Clausen, M.; Dalesio, J. The experimental physics and industrial control system architecture: Past, present, and future. *Nucl. Instrum. Methods Phys. Res. A* **1994**, *352*, 179–184. [\[CrossRef\]](#)
5. Nkadameng, E.K.; Gololo, M.; Karmoude, M.; Stodart, N.; Kumar, M.; Mellado, B. Vanilla LSTM Predictive Maintenance Model for Scientific Research Facilities. *Sensors* **2026**, *in press*. [\[CrossRef\]](#)
6. Mekki, K.; Bajic, E.; Chaxel, F.; Meyer, F. A comparative study of LPWAN technologies for large-scale IoT deployment. *ICT Express* **2019**, *5*, 1–7. [\[CrossRef\]](#)
7. Semtech Corporation. *AN1200.22 LoRa Modulation Basics*; Application Note; Semtech: Camarillo, CA, USA, 2019.
8. Boukabache, H.; Danzeca, S.; Heracleous, N.; Perrin, D.; Pirc, V.; Zimmario, A.; Murtas, F.; Silari, M. An IoT LoRaWAN network for environmental radiation monitoring at CERN. *IEEE Trans. Instrum. Meas.* **2021**, *70*, 6008512. [\[CrossRef\]](#)
9. ANSI/VITA. *VMEbus International Trade Association Standard 1-2014*; VITA: Scottsdale, AZ, USA, 2014.
10. OPC Foundation. *OPC Unified Architecture Specification, Part 1: Overview and Concepts*; Release 1.04; OPC Foundation: Scottsdale, AZ, USA, 2017.
11. ATLAS Collaboration. Operation of the ATLAS trigger and data acquisition system in LHC Run 3. *J. Instrum.* **2022**, *17*, P10038. [\[CrossRef\]](#)
12. 3GPP. *Technical Specification 36.201: LTE Physical Layer, Release 13*; 3GPP: Sophia Antipolis, France, 2016.
13. Sigfox. *Sigfox Technical Overview*; White Paper; Sigfox: Labège, France, 2017.
14. Adam, R.; Antel, C.; Bashir, M.; Benchekroun, D.; Bertou, X.; Böttcher, M.; Buffler, A.; Chen, A.; Essig, R.; Gascon, J.; et al. Paarl Africa Underground Laboratory (PAUL). *arXiv* **2023**, arXiv:2306.12083. [\[CrossRef\]](#)

15. IEC 61000-6-2; Electromagnetic Compatibility (EMC) Part 6-2: Generic Standards Immunity for Industrial Environments. International Electrotechnical Commission: Geneva, Switzerland, 2016.
16. Arksey, H.; O'Malley, L. Scoping studies: Towards a methodological framework. *Int. J. Soc. Res. Methodol.* **2005**, *8*, 19–32. [[CrossRef](#)]
17. Peters, M.D.J.; Godfrey, C.M.; Khalil, H.; McInerney, P.; Parker, D.; Soares, C.B. Chapter 11: Scoping Reviews. In *JBI Manual for Evidence Synthesis*; Aromataris, E., Munn, Z., Eds.; JBI: Adelaide, Australia, 2020.
18. Tricco, A.C.; Lillie, E.; Zarin, W.; O'Brien, K.K.; Colquhoun, H.; Levac, D.; Moher, D.; Peters, M.D.; Horsley, T.; Weeks, L. PRISMA Extension for Scoping Reviews (PRISMA-ScR): Checklist and explanation. *Ann. Intern. Med.* **2018**, *169*, 467–473. [[CrossRef](#)] [[PubMed](#)]
19. Munn, Z.; Peters, M.D.; Stern, C.; Tufanaru, C.; McArthur, A.; Aromataris, E. Systematic review or scoping review? Guidance for authors when choosing between a systematic or scoping review approach. *BMC Med. Res. Methodol.* **2018**, *18*, 143. [[CrossRef](#)] [[PubMed](#)]
20. Boukabache, H.; Danzeca, S.; Heracleous, N.; Perrin, D.; Pirc, V.; Zimmaro, A.; Murtas, F.; Silari, M. Monitoring particle accelerators with wireless IoT. In *Proceedings of the 12th International Beam Instrumentation Conference (IBIC 2023), Saskatoon, SK, Canada, 10–14 September 2023*; CERN: Geneva, Switzerland, 2023.
21. Srour, J.R.; Marshall, C.J.; Marshall, P.W. Review of displacement damage effects in silicon devices. *IEEE Trans. Nucl. Sci.* **2003**, *50*, 653–670. [[CrossRef](#)]
22. Chehri, A.; Fortier, P.; Tardif, P.M. UWB-based sensor networks for localisation in mining environments. *Ad Hoc Netw.* **2009**, *7*, 987–1000. [[CrossRef](#)]
23. IEC 61508-1:2010; Functional Safety of E/E/PE Safety-Related Systems—Part 1: General Requirements. IEC: Geneva, Switzerland, 2010.
24. Warden, P.; Situnayake, D. *TinyML: Machine Learning with TensorFlow Lite on Arduino and Ultra-Low-Power Microcontrollers*; O'Reilly Media: Sebastopol, CA, USA, 2020.
25. Banbury, C.R.; Reddi, V.J.; Lam, M.; Fu, W.; Fazel, A.; Holleman, J.; Huang, X.; Hurtado, R.; Kanter, D.; Lokhmotov, A.; et al. Benchmarking TinyML systems: Challenges and direction. *arXiv* **2021**, arXiv:2003.04821.
26. IEEE Std 802.15.4z-2020; Amendment to IEEE Std 802.15.4 Enhanced Ultra-Wideband (UWB) Physical Layers (PHYs) and Associated Ranging Techniques. IEEE Standards Association: Piscataway, NJ, USA, 2020.
27. Ericsson. *Ericsson Mobility Report, November 2024*; Ericsson: Stockholm, Sweden, 2024.
28. Easterbrook, P.J.; Berlin, J.A.; Gopalan, R.; Matthews, D.R. Publication bias in clinical research. *Lancet* **1991**, *337*, 867–872. [[CrossRef](#)] [[PubMed](#)]

Disclaimer/Publisher's Note: The statements, opinions and data contained in all publications are solely those of the individual author(s) and contributor(s) and not of MDPI and/or the editor(s). MDPI and/or the editor(s) disclaim responsibility for any injury to people or property resulting from any ideas, methods, instructions or products referred to in the content.